buy on www.cablematic.com

TENMARS

RF three-Axle Field Strength Meter

User's Manual



CE

HB2TM1950002

buy on www.cablematic.com

Table of Contents

1 Introduction 1
2 Simple a method of operation 1
3 Fundamentals 1
3.1 Electric field strength (E): 1
3.2 Magnetic field strength (H): 1
3.3 Power density (S): 2
3.4 The characteristic of electromagnetic fields: 2
4 Application 3
5 Features 4
6 Identifying Parts 5
7 LCD description 6
8 Specifications 7
8.1 General specifications 7
8.2 Electrical specifications 8
8.3 Units of measurement 9
8.4 Result modes 9
9 Measurement Procedures and Preparation 10
9.1 POWER button： 10
9.2 Data hold button: 10
9.3 Units button: 10
9.4 MAX / AVG Record: 11
9.5 Manual data memory storing 11
9.6 Backlight Display and Reading in The Dark. 11
9.7 XYZ/CALL: 12
9.8 Alarm ON/OFF Setup 12
9.9 Viewing Data Records 12
9.10 Clock LCD Display 13
10 Setup Mode 14
10.1 Clock Setup-1 14
10.2 Setting the alarm limit value (ALARM)-2 15
10.3 DEL data logger memorysetup-3 15
10.4 Analogue bar graphsetup-4 16
10.5 Auto Power Off Time function setup-5 16
10.6 Setting the calibration factor (CAL)-6 17
11 Making measurements 18
12 Short-term measurements 18
13 Long-term exposure measurements 19
14 SAFETY INFORMATION 19
15 SAFETY INFORMATION 20
16 Battery replacement 21
17 Safety Precaution 21
18 End of life 21

1 Introduction

This meter is designed for measuring and monitoring Radio–Frequency electromagnetic field strength. The meter is calibrated precisely over the frequency range of 50Mz~3.5 GHZ.

2 Simple a method of operation

Press  button to power on. To change measuring unit (mV/m), push ""button to change the unit.Electric field strength (V/m).Computed magnetic field strength (mA /m). Computed power density (mW/m^2).Computed power density (μW/cm^2).

Press  this key to change sensor axis selector :"All axis" → "X axis "→ "Y axis" → "Z axis".

3 Fundamentals

Electromagnetic pollution:

This meter is used to indicate electromagnetic pollution generated artificially. Wherever there is a voltage or a current, electric (E) and magnetic (H) fields arise. All types of radio broadcasting and TV transmitters produce electromagnetic fields, and they also arise in industry, business and the home, where they affect us even if our sense organs perceive nothing.

3.1 Electric field strength (E):

A field vector quantity that represents the force (F) on an infinitesimal unit positive test charge (q) at a point divided by that charge. Electric field strength is expressed in units of volts per meter (mV/m). This meter measures electric field strength directly.

3.2 Magnetic field strength (H):

A field vector that is equal to the magnetic flux density divided by the permeability of the medium. Magnetic field strength is expressed in units of amperes per meter (A/m). In far field

situations, one can calculate the magnetic f-ield for the electric field value. This meter can display the calculated magnetic field strength.

3.3 Power density (S):

Power per unit area normal to the direction of propagation, usually expressed in units of watts per square meter (W/m^2) or, for convenience, units such as mill watts per square centimeter (mW/cm^2).

3.4 The characteristic of electromagnetic fields:

Electromagnetic fields propagate as waves and travel at the speed of light (C). The wavelength is proportional to the frequency.

λ (wavelength) = C (speed of light) / f (frequency)

If the distance to the field source is less than three wavelengths, then we are usually in the near field. If the distance is more than three wavelengths, the far-field conditions usually hold.
In near field conditions, the magnetic field value cannot be calculated from the electric field value. This meter is designed for reliable far field measurements only.

buy on www.cablematic.com

4 Application


- Quite often routine, maintenance and service work has to be done in areas where active electromagnetic fields are present, e.g. in broadcasting stations, etc. Additionally, other employees may be exposed to electromagnetic radiation. In such cases, it is essential that personnel be not exposed to dangerous levels of electromagnetic radiation, such as:
- High frequency(RF)electromagnetic wave field strength measurement.
- Mobile phone base station antenna radiation power density measurement.
- Wireless communication applications (CW, TDMA, GSM, DECT).
- RF power measurement for transmitters.
- Wireless LAN (Wi-Fi) detection, installation.
- Spy camera, wireless bug finder.
- Cellular /Cordless phone radiation safety level. Microwave oven leakage detection.
- Personal living environment EMF safety.

buy on www.cablematic.com

5 Features


- The meter is a broadband device for monitoring high-frequency radiation in the range from 50MHz to 3.5GHz
- The non-directional electric field antenna and high sensitivity also allow measurements of electric field strength in TEM cells and absorber rooms.
- The unit of measurement and the measurement types have been selected to expressed in units of electrical and magnetic field strength and power density.
- At high frequencies, the power density is of particular significance. It provides a measure of the power absorbed by a person exposed to the field. This power level must be kept as low as possible at high frequencies.
- The meter can be set to display the instantaneous value, the maximum value measured or the average value. Instantaneous and maximum value measurements are useful for orientation, e.g. when first entering an exposed area.
- For isotropic measurements of electromagnetic fields.
- Non-directional (isotropic) measurement with three-channel measurement sensor.
- High dynamic range due to three- channel digital results processing.
- Configurable alarm threshold and memory function.
- Easy & safe to use
- Low battery detector "".
- Over load indication "OL".

6 Identifying Parts

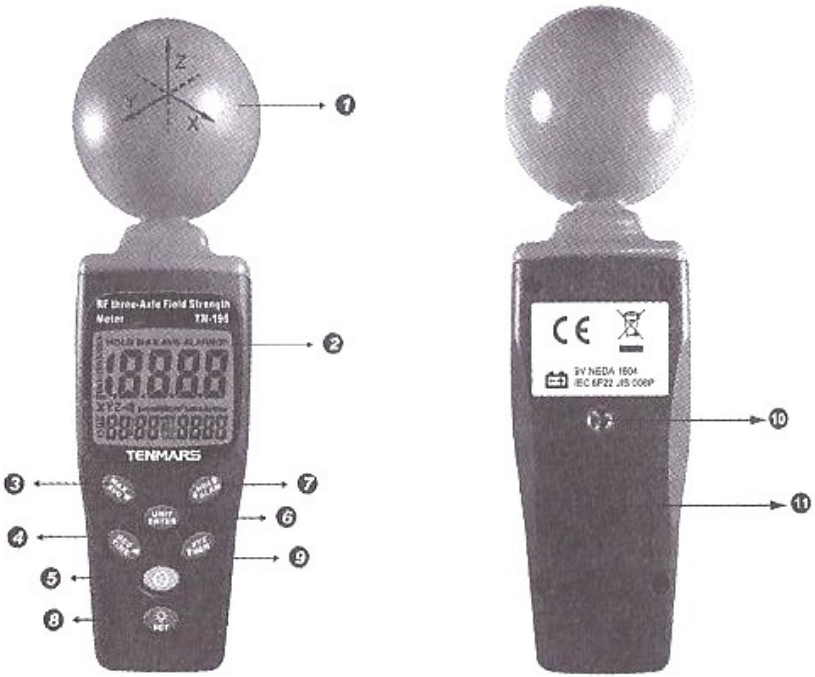

1. RF three-Axle Sensor.
2. Liquid-crystal LCD.
3. MAX / AVG / R Button.
4. Record / Time / L Button.
5. Power Button.
6. UNIT / ENTER switch Button.
7. Hold / Up Button.
8. Backlight/Set
9. XYZ / MEM / Down Button.
10. Tripod mounting screw.
11. Battery cover.

7 LCD description

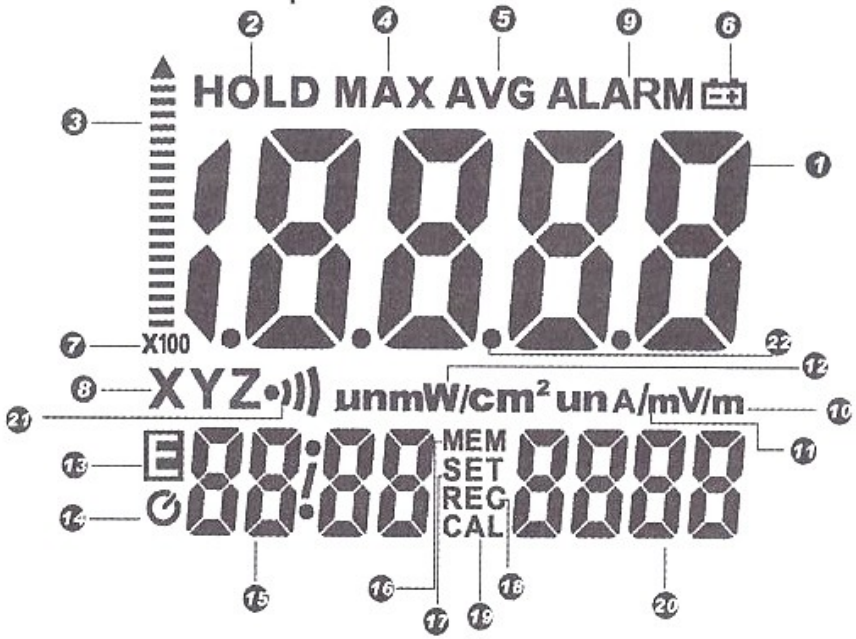

1. Primary Display
2. Hold symbol
3. Analogue bar graph
4. MAX symbol
5. AVG symbol
6. Low battery symbol
7. x1x10x100 unit
8. X.Y.Z unit
9. ALARM unit
10. mV/m,V/m (E)
11. µA/m mA /m unit (H)
12. µW/m, µW/cm^{2}unit
13. E symbol
14. Auto power off symbol
15. Time unit (month:day) (hour: minute) (second)
16. MEM reading symbol
17. SET symbol
18. REC symbol
19. CAL symbol
20. Secondary Display
21. BUZZER symbol
22. Decimal point

buy on www.cablematic.com

8 Specifications

8.1 General specifications

- Display type: Liquid-crystal (LCD), 4-1/2 digits maximum reading 19999.
- Measurement method: Digital, triaxial measurement.
- Directional characteristic: Isotropic, triaxial.
- Measurement range selection: one continuous range.
- Display resolution:0. 1mV/m, 0.1μA/m, 0.001μW/m2, 0.001μW/cm2
- Setting time: typically 1.5s (0 to 90% measurement value.)
- Sample rate:3 times per second.
- Audible alarm: Buzzer.
- Units: mV/m, V/m, μA/m, mA/m, μW/m2, mW/m2, μW/cm2
- Display value: Instantaneous measured value, maximum value, average value, or maximum average value.
- Alarm function: adjustable threshold with ON / OFF
- Calibration factor CAL: adjustable
- Manual data memory and read storage:200 data sets.
- Batteries: 9V NEDA 1604, IEC 6F22 or JIS 006P
- Battery life: Approximate 15 hours.
- Auto power off: Default time 15 minutes. Adjustable threshold 0~99 minutes.
- Operating temperature range: 0°C to + 50°C
- Operating humidity range: 25% to 75 % RH
- Storage temperatures range: -10°C to +60°C
- Storage humidity range: 0% to 80% RH
- Dimensions: 60(L)*60(W)*195(H) mm.
- Weight (including battery): Approx.200g.
- Accessories: User's manual, 9V battery, Carrying case.

EMC

This tester was designed in accordance with EMC Standards in force and its compatibility has been tested in accordance with EN61326-1 (2006).

8.2 Electrical specifications

- Unless otherwise stated, the following specifications hold under the following conditions:
- The meter is located in the far field of a source; the sensor head is pointed towards the source.
- Ambient temperature: +23 °C ±3°C.
- Relative air humidity 25%~75%

- Sensor type: electrical field (E).
- Frequency range: 50MHz ~ 3.5GHz.
- Specified measurement range:
  CW signal (f >50MHz):38mV/m to 20.00 V/m, 53.0uA/m to 53.74mA/m 0.1uW/m^2 1.089W/m^2, 0.001uW/cm^2~108.9uW/cm^2
- Dynamic range: Typically 75dB
- Absolute error at 1V/m and 50 MHz.

12. Frequency response:

- Sensor taking into account the typical CAL factor:
- ± 2.4dB (50 MHz to 1.9 GHz).
- ±1.0 dB (1.9 GHz to 3.5GHz).
- Isotropy deviation: Typically ± 1.0 dB (f 2.45GHz).
- Overload limit: 0.42 mW/cm^2 (11 V/m) per axis.
- Overload limit: (0 to50°C): ± 0.2dB.

buy on www.cablematic.com

8.3 Units of measurement


The meter measures the electrical component of the field; the default units are those of electrical field strength (mV/m or V/m). The meter converts the measurement values to the other units of measurement, i.e. the corresponding magnetic field strength units (μA/m or mA/m) and power density units (μW/m^2 , mW/m^2 or μW/cm^2) using the standard far-field formulate for electromagnetic radiation.
The conversion is invalid for near-field measurements, as there is no generally valid relationship between electrical and magnetic field strength in this situation. Always use the default units of the sensor when making near-field measurements.

8.4 Result modes

The bar graph display always shows the instantaneous measured dynamic range value. The digital display shows the result according to one of three modes, which can be selected.

Instantaneous: The display shows the last value measured value measured by the sensor, no symbol is displayed.
Maximum instantaneous (MAX):The digital display shows the highest instantaneous value measured, the “MAX “symbol is displayed.

Average (AVG): The digital display shows the average value measured, the “AVG” symbol is displayed.
Instantaneous mode is the default setting when the meter is turned on. The following graph shows of Instantaneous (actual), MAX (hold), AVG and MAX/AVG:

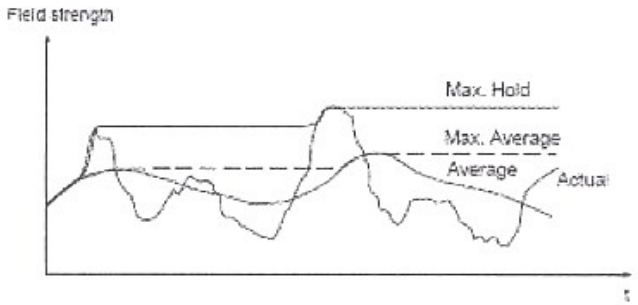

9 Measurement Procedures and Preparation

Battery loading: Remove the battery cover on the back and put a 9V battery inside.

Battery replacement: When the symbol of “ ” appears on the LCD display, the battery should be replaced with a new one. The battery symbol will be displayed on the LCD, this is a battery low indicator.

9.1 POWER button :

Press button to power on. Again

Press button to power off.

9.2 Data hold button:

Press the “ ” button to go into hold mode, and “HOLD” appears on the screen to allow you to read the data.

Press “ ”this button once again to deactivate it.




buy on www.cablematic.com

9.3 Units button:

Change units with the “UNITS” key as follows.
Electric field strength (V/m)
Computed magnetic field strength (mA/m).
Computed power density (mW/m^2).
Computed power density (μW/cm^2).

Press “ ” button and push “ ”button to change the unit.
Possible units: mV/m, V/m, μA/m , mA/m, μW/m^2, mW/m^2, μW/cm^2

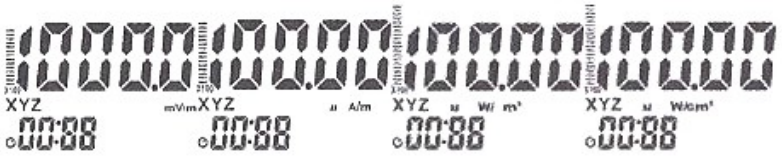

9.4 MAX / AVG Record:

Press "MAX AVG" key to switch to the next display. The display switches from MAX to AVG to MAX/AVG and back to MAX.



Press and hold "MAX AVG" key for 3 seconds to disable this function.
The maximum storage is up to 99 minutes and 99 seconds
After this period of time, updating will be completed automatically and then the LCD displays .

9.5 Manual data memory storing

Push "REC UNIT" button, the meter will save the current measured result, and REC with a number 001~200 will appear.
Manual data memory storing: 200 data sets.
Over load indication: "OL".




9.6 Backlight Display and Reading in The Dark.

Press "☼" key backlight light on. Again Press ☼ button to power off.
Backlight light turns off automatically after 30 seconds.


9.7 XYZ/CALL:

Press XYZ MEM this key to change sensor axis selector :"All axis" → "X axis "→ "Y axis" → "Z axis".

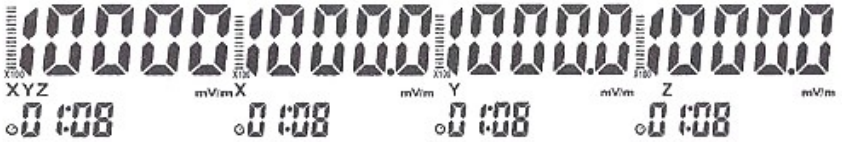

9.8 Alarm ON/OFF Setup

Press hold ① and HOLD ALARM key to switch the alarm function on The "ALARM" symbols in the display indicates that the alarm function is on. Press hold ① and HOLD ALARM key to turn off the alarm function. When the Alarm sounds, the display shows .

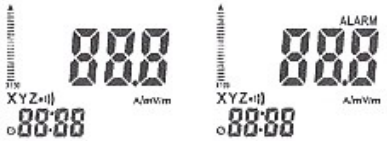

9.9 Viewing Data Records

Press hold "①"button and press"XYZ MEM"button to view the saved data records
Use "HOLD ALARM" or "XYZ MEM" button to see the next or previous records
Press UNIT ENTER key to close the setup, exit the mode.



buy on www.cablematic.com

9.10 Clock LCD Display

Press hold [ ] and [REC TIME] button to select the display method of the Year, Month, Date, hour and Second.
This meter's clock uses 24 hour time setting.
Default time mode setting is “2010/01/07 00: 02” “:00”.



buy on www.cablematic.com

10 Setup Mode

Press hold “[ ]” button and “[SET]” button to enter the setup mode.

Press “[SET]” button to change the setup function. (Setup function see Note1)

Push “[UNIT ENTER]” button to save setup data
Note1: you can set up 6 different functions in setup mode
Clock Setup
setup 1 : Setting the alarm limit value (ALARM)
setup 2 : Clear data logger memory
setup 3 : Analogue bar graph X1.X10.X100
setup 4 : Auto Power Off Time
setup 5 : Setting the calibration factor (CAL)

10.1 Clock Setup-1

Press hold “[ ]” button and press “[SET]” button first to enable Clock Setup
This meter clock is 24 hour time setting.

Use “[HOLD ALM]” or “[MAX MIN]” to change digit(Hour→day→Month→year →Minute).

Use “[REC TIME]” or “[MAX AVG]” to select the digit you want to adjust.

Press “[UNIT ENTER]” button to save the setting.
Date/Time default format:2009/12/21 12:12.
Year format: 2000~2099 display as 00 ~ 99.



10.2 Setting the alarm limit value (ALARM)-2

The alarm limit value is used to monitor the display value automatically. It controls the alarm indication function. The alarm limit value can be edited in the displayed V/m unit. The ALARM setting range is from 0.001 to 999.9V/m. ALARM default is set at 999.9V/m.
Alarm limit function is only used for total three axial value comparator.

Press and hold on "" button and press "SET" button to enter Setup Mode.

then press SET button 1 more time to enter the alarm setting mode, the "V/m" unit is flashing displayed.

Press "" key to move decimal.

Press "REC TIME" key to select the desired setting value.

Press "HOLD ALAM" and "XYZ MEM" button to change digit.

Press "UNIT ENTER" key to store the new setting value and exit.



10.3 DEL data logger memorysetup-3

Press and hold on "" button and press "SET" button to enter Setup Mode.

Press "SET" button 2 more times to enter clear data logger memory mode (3.SET).



Press" XYZ MEM key in the display "SET 000 ' Press UNIT ENTER key Will exit and not clear memory.

buy on www.cablematic.com



Press" HOLD ALAM key to display "SET 000'. Press "UNIT ENTER" key to exit without clearing the data.

10.4 Analog bar graph setup-4

Press hold "" button and press "SET" button to enter Setup Mode.

Press SET button 3 more times to: Analogue bar graph setting mode. The " graph" unit is flashing displayed X1、X10、X100.

Press"HOLD ALAM" "and " "XYZ MEM" to select the desired setting value X1 、X10 、X100。



Press "UNIT ENTER" key to store the new setting value and exit.

10.5 Auto Power Off Time function setup-5

If you want to disable auto power off, please hold "" button and press "SET" 、 button to enter Setup Mode.

Press "SET" button 4 more times.

Press "HOLD ALAM "and "XYZ MEM" button to change digit. Set value to 00 to disable auto power off.

Press "UNIT ENTER" key to store the new setting value and exit.the symbol ⏲ is displayed.
Maximum auto power off time:00~99 minutes.
Auto power off time default setting is 15 minutes.



10.6 Setting the calibration factor (CAL)-6


please hold " " button and press " " button to Setup Mode

press " " button 5 more times to turn on the meter to enter the calibration factor, The CAL setting range is from 0.10 to 9.99.

Press " " and " " button to change digit

Use " " or " " to select the desired setting value.
on the meter to enter the calibration factor setting mode, the " CAL SET " marks is displayed.

Press " " key to store the new setting value and exit.

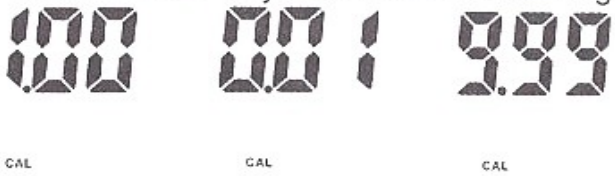

Calibration factor (CAL)
The calibration factor CAL serves to calibrate the result display. The field strength value measured internally is multiplied by the value of CAL that has been entered and the resulting value is displayed. The CAL setting range is from 0.10 to 9.99.
The CAL factor is often used as a means of entering the sensitivity of the field sensor in terms of its frequency response in order to improve measurement accuracy.

11 Making measurements

Important:
The following effect will be noted with all field strength meters: If the sensor is moved quickly, excessive field strength values could be displayed. This effect is caused by electrostatic charges.
Recommendation:
Hold the meter steady during the measurement.

12 Short-term measurements

Application:
Use either the "instantaneous" or the "Max. instantaneous" mode, if the characteristics and orientation of the field are unknown when entering an area exposed to electromagnetic radiation.
Procedure:
Hold the meter at arm's length.
Make several measurements at various locations around your work place or the interested areas as described above. This is particularly important is the field conditions are unknown.
Pay special attention to measuring the vicinity of possible radiation sources. Apart from active sources, those components connected to a source may also act as radiators. For example , the cables used in diathermy equipment may also radiate electromagnetic energy. Note that metallic objects within the field may locally concentrate or amplify the field from a distant source.

buy on www.cablematic.com

13 Long-term exposure measurements

Location

Place the meter between yourself and the suspected source of radiation. Make measurements at those points where parts of your body are nearest to the source of radiation.

Note: Use the “Average” or” Max average” modes only when the instantaneous measurement values are fluctuating greatly.

You may fix the meter to a wooden or plastic tripod.

14 SAFETY INFORMATION

CAUTION

Before making a measurement, check if the low battery symbol”  ” is shown on the display as soon as the meter is switched on. Change the battery if the symbol is displayed.

In the case of prolonged storage, it is preferable to remove the battery from the meter.

Avoid shaking the meter, particularly in the measurement mode.

The specified limits outside and improper handling may adversely affect the accuracy and function of the meter.

buy on www.cablematic.com

15 SAFETY INFORMATION

DANGER

In some cases, work in the vicinity of powerful radiation sources can be a risk of your life.

Be aware that persons with electronic implants (e.g. cardiac pacemakers) are subject to particular dangers in some cases.

Observe the local safety regulations of the facility operation.

Observe the operating instructions for equipment, which is used to generate, conduct, or consumer electromagnetic energy.

Be aware that secondary radiators (e.g. reflective objects such as a metallic fence) can cause a local amplification of the field.

Be aware that the field strength in the near vicinity of radiators increases proportionally to the inverse cube of the distance. This means that enormous field strengths can result in the immediate vicinity of small radiation sources (e.g. leak in wave guides, inductive ovens)

Field strength measuring device can underrate pulsed signals. Particularly with radar signals, significant measurement errors can arise.


All field strength measuring devices have a limited specified frequency range. Fields with spectral components outside of this frequency range are generally incorrectly evaluated and tend to be underrated. Before using field strength measuring devices, you should thus be certain that all field components to be measured lie in the specified frequency range of the measuring device.

16 Battery replacement

WARNING

If the symbol " [-+] " appears on the LCD, please replace the battery immediately

- Turn off the instrument.
- Remove the battery cover
- Replace the battery.
- Install the battery cover.

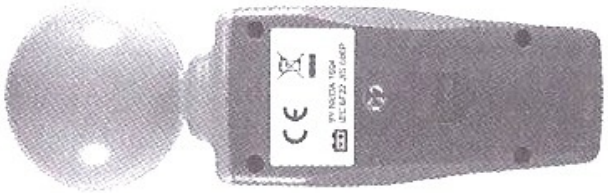

17 Safety Precaution

- For cleaning the instrument use a soft dry cloth. Never use a wet cloth, solvents or water, etc..
- Operation Altitude: Up to 2000M.
- Operating Environment: Indoors use. This instrument has been designed for being used in an environment of pollution degree 2.

18 End of life



Caution: this symbol indicates that equipment and its accessories shall be subject to a separate collection and correct disposal

buy on www.cablematic.com